

## UV4C-H Ultraviolet Disinfection Cabinet




**59 L**

Big enough to disinfect  
multiple items  
Small enough to fit your places

**10**  
minutes

Proven to inactivate Covid-19.

### Features

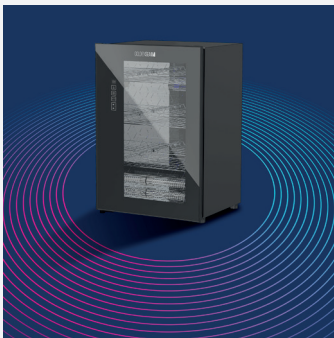


#### Safety by design

When the door is opened, the built-in sensor will immediately deactivate the lamp



#### Buzzer alarm

indicates the end of disinfection  
Can adjust the volume at will,  
suitable for different places

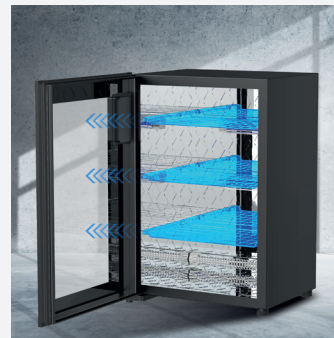

#### 3 removables shelves

For maximum flexibility



#### No Ozone

Safe and harmless – Leave no residue

Note: Only when used in accordance with  
manufacturer instructions



**High quality lamp / Quartz glass tube**  
Allows full transmission of ultraviolet light




#### Only 30 W

Other units normally require 300-500 W



#### 6,000 hours long life tubes

Up to 36,000 times of use

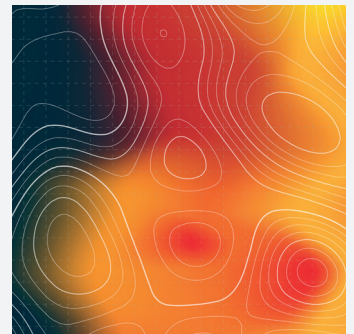


#### Heating Functionality (optional)

Dry your devices while disinfecting



## Application areas

Mobile phones, headsets, masks, office supplies, cosmetic tools, baby supplies, etc.

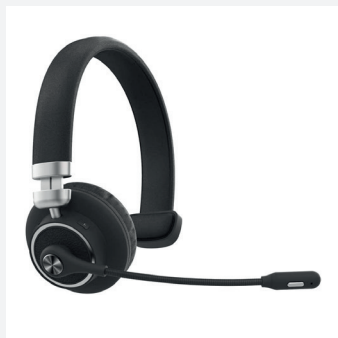

## Product information

**Product:** GOLDENSEA UV Ultraviolet Disinfection cabinet  
**Model:** UV4C-H  
**Light Source Wattage:** 4W x 2  
**Light Source Lifespan:** Max. 6,000h  
**Voltage:** 100VAC~120VAC 50/60HZ & 220~240VAC 50/60HZ

**Control:** Touch keys  
**Material:** aluminum alloy and anti-UV organic glass  
**Function:** UV disinfection  
**Wavelength:** 253.7 nm  
**Product dimension:** 440 x 370 x 650 mm  
**Weight:** 12.3kg

**Cable Length:** 1.8m  
**Compliance:** CE, REACH  
**Application:** Disinfect daily use items: mobile phone, headset, mask, office stationery, makeup tools, and other items



## Warning

Ultraviolet light can cause damage to eyes and skin.  
All personnel, animals and plants must leave/ be moved from the site during use.

## Precautions

1. The disinfection function can only be activated after the cabinet door is closed.

2. Valuables are not recommended to be put into the cabinet. Items may be discolored.

3. Inflammable and explosive articles are prohibited to be put into the disinfection cabinet.